


VERIFICATION OF CALIBRATION REPORT
Of Data-Master cdm Breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program


Data-Master cdm S/N: 130296 ✓		
Supervisor/Operator Performing the Verification Procedure:		
Name <u>John J. Waldron</u> ID: # <u>3392 ✓</u> Date: <u>01/29/11 ✓</u>		
A. Agency <u>Unalaska Department of Public Safety</u> Phone <u>907-581-1233</u>		
Instrument Location <u>Unalaska Department of Public Safety, PO Box 370, 29 Safety Way, Unalaska, AK 99685</u>		
Alco S/N: <u>78966 ✓</u> Target Value: <u>.082 ✓</u> High Pressure: <u>200</u>		
B. Alco Test Values		
	<u>.082 ✓</u> 1 st Test Value	<u>.083 ✓</u> 2 nd Test Value
Signature <u></u>		
(OVER)		

(Do not write in the area below)


JMB
2/8/11


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

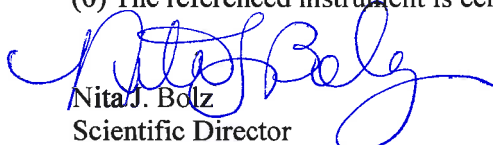
Nita J. Bolz
Scientific Director

State Breath Alcohol Program
Subscribed and sworn before me this 14th day of MAR, 2011.

 (Notary Seal Stamp)
Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT
Of Data-Master cdm Breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory -- Statewide Breath Alcohol Program

Data-Master cdm S/N: 130296

Supervisor/Operator & Number Performing the Verification Procedure: John J. Waldron, #3392
Department and Date: Unalaska DPS

(CONTINUED FROM FRONT PAGE)

**C. TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE
DIAGNOSTIC CHECK IN THE MARKED BOXES.**

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130296

JANUARY 29, 2011

OPERATOR'S NAME:

WALDRON/JOHN/J

OPERATOR'S NUMBER: 3392

SUBJECT'S LAST NAME:

UOC

SUBJECT'S FIRST NAME/MI :

UOC

D.L. #: 0123456789

DEPT/AGENCY: UNK1

CASE/REPORT: 11-00000

TEST TYPE: U

ALCO TARGET VALUE: .002

ALCO S/N: 78966

--- BREATH ANALYSIS ---

.002 ADJUSTED FOR 29.33 in		
ALCO TARGET	.000	03:47
BLANK TEST	.000	03:48
INTERNAL STANDARD	VERIFIED	03:48
ALCO TU 29.33 in	.002	03:48
BLANK TEST	.000	03:49
SUBJECT SAMPLE	.000	03:50
BLANK TEST	.000	03:50
ALCO TU 29.33 in	.003	03:51
BLANK TEST	.000	03:51

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130296

JANUARY 29, 2011

TIME 03:53

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	40c
BREATH TUBE:	40c
BAROMETER:	29.33 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#\$%^&*+,-./0123456789:;<=>?@ABCDEF6
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmnop
qrstuvwxyz{|}~